



# Certificate of Analysis

Apr 10, 2020 | zephyr health products

289 route 33 east,  
Manalapan , NJ, 07726, USA

Sample: DA00409004-001  
Harvest/Lot ID: 103  
Batch#: 103a  
Seed to Sale# N/A  
Batch Date: N/A  
Sample Size Received: 15 ml  
Total Batch Size: 30 ml  
Retail Product Size: 30 ml gram  
Ordered : 03/12/20  
Sampled : 03/12/20  
Completed: 04/10/20  
Sampling Method: SOP.T.20.010.FL

**PASSED**

Page 1 of 1



PRODUCT IMAGE




30ml blue tincture with white eyedropper cap

SAFETY RESULTS

								
Pesticides NOT TESTED	Heavy Metals NOT TESTED	Microbials NOT TESTED	Mycotoxins NOT TESTED	Residuals Solvents NOT TESTED	Filth NOT TESTED	Water Activity NOT TESTED	Moisture NOT TESTED	Terpenes NOT TESTED

MISC.

 **Cannabinoid** **PASSED**

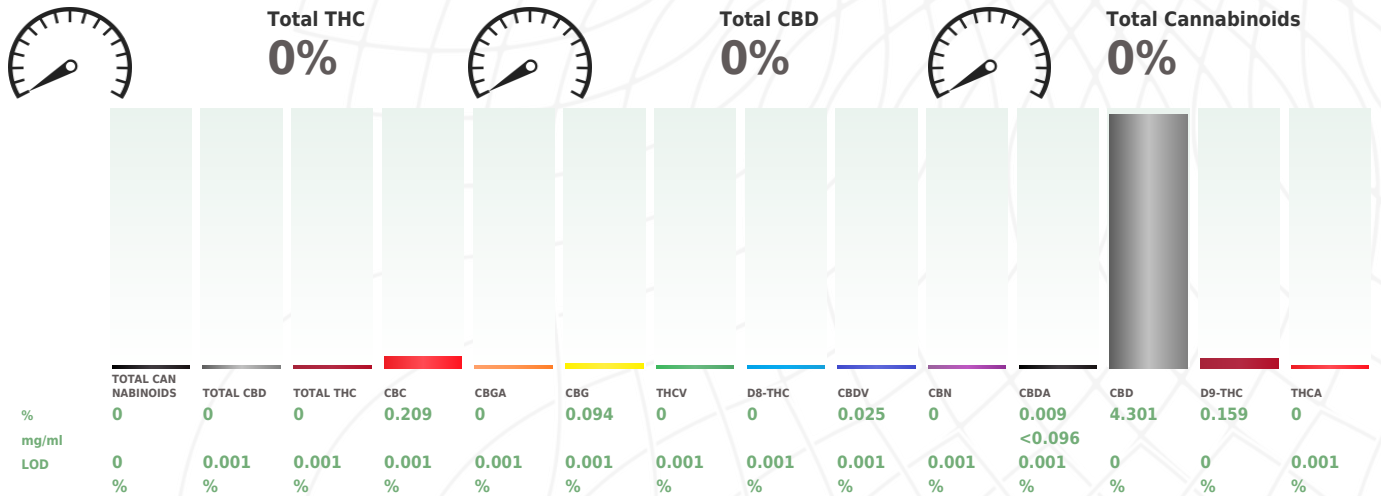

Analyzed by: 450      Weight: 3.0517g      Extraction date: 04/09/20 09:04:09      Extracted by: 965

Analysis Method : SOP.T.40.031, SOP.T.30.031  
Analytical Batch : DA011541POT  
Instrument Used : DA-LC-003  
Running on : N/A

Dilution : 400  
Reagent : 032320.30; 040720.R18; 040720.R17  
Consumables : 180111; 914C4-914AK; 929C6-929H  
Pipette : N/A

Reviewed On : 04/10/20 10:48:32  
Batch Date : 04/09/20 08:27:57

Full Spectrum cannabinoid analysis utilizing High Performance Liquid Chromatography with UV detection in accordance with F.S. Rule 64ER20-39.

This Kaycha Labs Certification shall not be reproduced, unless in its entirety, without written approval from Kaycha Labs. The results relate only to the material or product analyzed. ND=Not Detected, ppm=Parts Per Million, ppb=Parts Per Billion, RSD=Relative Standard Deviation, Limit of Detection (LOD) and Limit Of Quantitation (LOQ) are terms used to describe the smallest concentration that can be detected and reliably measured by an analytical procedure, respectively. Action Levels are State determined thresholds based on F.S. Rule 64ER20-39 and F.S. Rule 5K-4. The Measurement of Uncertainty (MU) error is available from the lab upon request. The "Decision Rule" for pass/fail does not include the MU. Any calculated totals may contain rounding errors.

**Jorge Segredo**  
Lab Director

State License # CMTL-0002  
ISO Accreditation # ISO/IEC  
17025:2017 Accreditation PJLA-  
Testing 97164

  
Signature

04/10/20

Signed On